



## User's Manual

# KLH IgM (Human) ELISA Kit

REF

DEIA-BY028



96T

RUO

This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

---

### Creative Diagnostics

 Address: 45-1 Ramsey Road, Shirley, NY 11967, USA

 Tel: 1-631-624-4882 (USA) 44-161-818-6441 (Europe)  Fax: 1-631-938-8221

 Email: [info@creative-diagnostics.com](mailto:info@creative-diagnostics.com)  Web: [www.creative-diagnostics.com](http://www.creative-diagnostics.com)

---

## PRODUCT INFORMATION

### Intended Use

This kit allows quantitative measurement of human anti-KLH IgM levels in serum, plasma, and other fluids.

### Principles of Testing

The assay uses KLH as capture reagent coated on microtiter wells, and horseradish peroxidase (HRP) conjugated anti-human IgM for detection. Standards and diluted samples are incubated in microtiter wells for 45 minutes. The wells are subsequently washed. HRP conjugate is added and incubated for 45 minutes. Anti-KLH IgM molecules are thus sandwiched between immobilized KLH and the HRP conjugate. The wells are then washed to remove unbound HRP-labeled antibodies. TMB is added and incubated for 20 minutes at room temperature. This results in the development of a blue color. Color development is stopped by the addition of stop solution, changing the color to yellow. Absorbance is measured at 450 nm. The concentration of anti-KLH IgM is proportional to the absorbance and is derived from a standard curve.

### Reagents And Materials Provided

1. KLH Coated 96-well plate (12 x 8 well strips)
2. Anti-Human IgM HRP Conjugate, 11 ml
3. Anti-KLH IgM Stock (lyophilized)
4. 20x Wash Solution, 50 ml
5. Diluent, 50 ml
6. TMB Reagent, 11 ml
7. Stop Solution (1N HCl), 11 ml

### Materials Required But Not Supplied

1. Precision pipettes and tips
2. Distilled or deionized water
3. Polypropylene or glass tubes
4. Vortex mixer
6. Absorbent paper or paper towels
7. Plate incubator/shaker with mixing speed of 150 rpm
8. Plate washer
9. Plate reader with an absorbance range of 0-4 at 450 nm
10. Graphing software

### Storage

The anti-KLH IgM stock should be stored at - 20°C or lower. The remainder of the kit should be stored at 4°C. The microtiter plate should be kept in a sealed bag with desiccant to minimize exposure to damp air. The kit will remain stable for six months from the date of purchase provided that the components are stored as described.

## Specimen Collection And Preparation

The optimal sample dilution should be determined empirically. Studies at Creative Diagnostics, using ascites fluid samples, suggest that a 500-fold dilution is a reasonable starting point.

## Reagent Preparation

1. All reagents should be allowed to reach room temperature (25°C) before use.
2. Optimal results are achieved if, at each step, reagents are pipetted into the wells of the microtiter plate within 5 minutes.
3. Wash Solution Preparation: The wash solution is provided as a 20x stock. Prior to use, dilute the contents of the bottle (50 ml) with 950 ml of distilled or deionized water.
4. Standard Preparation:
  - 1) Standards should be used within 30 min of preparation.
  - 2) The anti-KLH IgM stock is provided in lyophilized form. Reconstitute as directed on the vial label (the reconstituted stock should be frozen at - 20°C if additional use is intended).
  - 3) Label 6 polypropylene or glass tubes as 1000, 500, 250, 125, 62.5 and 31.25 ng/ml.
  - 4) Into the tube labeled 1000 ng/ml, pipette the volume of diluent detailed on the stock vial label. Then add the indicated volume of anti-KLH IgM and mix gently. This provides the 1000 ng/ml standard.
  - 5) Dispense 250 µl of diluent into the tubes labeled 500, 250, 125, 62.5 and 31.25 ng/ml.
  - 6) Prepare a 500 ng/ml standard by diluting and mixing 250 µl of the 1000 ng/ml standard with 250 µl of diluent in the tube labeled 500 ng/ml.
  - 7) Similarly prepare the remaining standards by serial dilution.

## Assay Procedure

1. Secure the desired number of coated wells in the holder.
2. Dispense 100 µl of standards and diluted samples into the wells.
3. Incubate on a plate shaker at 150 rpm/25°C for 45-minutes.
4. Aspirate the contents of the microtiter wells and wash the wells five times with 1x wash solution using a plate washer (400 µl/well).
5. Strike the wells sharply onto absorbent paper to remove all residual wash solution.
6. Add 100 µl of diluted HRP conjugate into each well.
7. Incubate on a plate shaker at 150 rpm/25°C for 45-minutes.
8. Wash as detailed above.
9. Dispense 100 µl of TMB into each well.




10. Incubate on a plate shaker at 150 rpm/25°C for 20-minutes.
11. Stop the reaction by adding 100 µl of stop solution to each well.
12. Gently mix. It is important to make sure that all the blue color changes to yellow.
13. Measure absorbance at 450 nm with a microtiter plate reader within five minutes.

## Calculation

1. Using graphing software construct a standard curve by plotting the absorbance of the standards versus concentration.
2. Fit standard data to a two-site, total and non-specific binding model (others may be used at the discretion of the researcher) and derive the concentration of anti-KLH IgM in the samples.
3. Multiply the derived concentration by the dilution factor(s) to determine the actual concentration of anti-KLH IgM in the original sample.
4. If absorbance values of samples fall outside the standard curve, samples should be diluted appropriately and re-tested.

## Typical Standard Curve

A typical standard curve is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns.

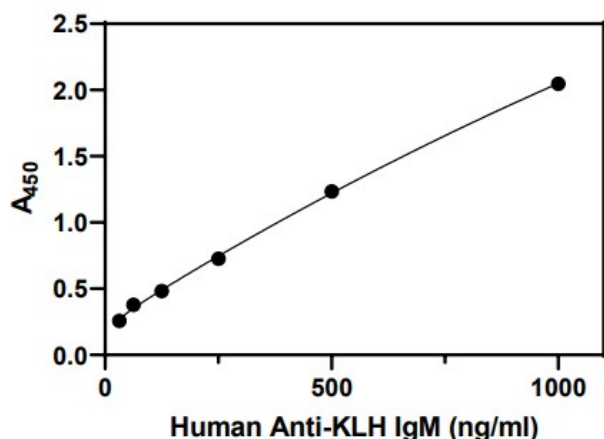

Anti-KLH IgM (ng/ml)	A <sub>450</sub>
1000	2.048
500	1.235
250	0.726
125	0.482
62.5	0.378
31.25	0.258

## Performance Characteristics

**Parallelism:** To assess performance of the assay, two samples containing anti-KLH IgM at concentrations of 58.5 and 8.7  $\mu\text{g/ml}$  were serially diluted from 50- to 1600-fold to produce values within the dynamic range of the assay.

