



## User's Manual

# cAMP ELISA Kit (For Acetylated and Non-acetylated cAMP)

REF

DEIA-CA01



96T

RUO

This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

---

### Creative Diagnostics

 Address: 45-1 Ramsey Road, Shirley, NY 11967, USA

 Tel: 1-631-624-4882 (USA) 44-161-818-6441 (Europe)  Fax: 1-631-938-8221

 Email: [info@creative-diagnostics.com](mailto:info@creative-diagnostics.com)  Web: [www.creative-diagnostics.com](http://www.creative-diagnostics.com)

---

## PRODUCT INFORMATION

### Intended Use

The cAMP assay is a competitive ELISA that permits cAMP measurements within the standard curve range of 0.078-10 pmol/ml, sensitivity (80% B/B<sub>0</sub>) of 0.1 pmol/ml for acetylated cAMP. Non-acetylated cAMP has a range from 0.3-750 pmol/ml and a sensitivity(80%B/B<sub>0</sub>) of approximately 3 pmol/ml.

### General Description

Adenosine 3',5' cyclic monophosphate (cAMP) is a ubiquitous cellular second messenger that is a critical component of a signal transduction pathway linking membrane receptors and their ligands to the activation of internal cellular enzymatic activity and gene expression. cAMP is synthesized from ATP by membrane-bound adenylate cyclase. Binding of ligands or hormones to their specific G protein-coupled receptors activates GTP binding proteins (G<sub>s</sub> or G<sub>i</sub>) which either stimulate or inhibit adenylate cyclase. cAMP activates or inhibits various enzymes or cascade of enzymes by promoting their phosphorylation or dephosphorylation. The cAMP signal is neutralized by hydrolysis of cAMP to AMP by phosphodiesterases. Therefore, the concentration of cAMP in a cell is a function of the ratio of the rate of synthesis from ATP by adenylate cyclase and its rate of breakdown to AMP by specific phosphodiesterases.

### Principles of Testing

This assay is based on the competition between free cAMP and a cAMP-acetylcholinesterase (AChE) conjugate (cAMP Tracer) for a limited number of cAMP-specific rabbit antibody binding sites. Because the concentration of the cAMP Tracer is held constant while the concentration of cAMP varies, the amount of cAMP Tracer that is able to bind to the rabbit antibody will be inversely proportional to the concentration of cAMP in the well. This rabbit antibody-cAMP (either free or tracer) complex binds to the mouse monoclonal anti-rabbit IgG that has been previously attached to the well. The plate is washed to remove any unbound reagents and then Ellman's Reagent (which contains the substrate to AChE) is added to the well. The product of this enzymatic reaction has a distinct yellow color and absorbs strongly at 412 nm. The intensity of this color, determined spectrophotometrically, is proportional to the amount of AMP Tracer bound to the well, which is inversely proportional to the amount of free cAMP present in the well during the incubation; or


$$\text{Absorbance} \propto [\text{Bound cAMP Tracer}] \propto 1/[\text{cAMP}]$$

The electric organ of the electric eel, *E. electricus*, contains an avid AChE capable of massive catalytic turnover during the generation of its electrochemical discharges. The electric eel AChE has a clover leaf-shaped tertiary structure consisting of a triad of tetramers attached to a collagen-like structural fibril. This stable enzyme is capable of high turnover (64,000 s<sup>-1</sup>) for the hydrolysis of acetylthiocholine.

A molecule of the analyte covalently attached to a molecule of AChE serves as the tracer in AChE enzyme immunoassays. Quantification of the tracer is achieved by measuring its AChE activity with Ellman's Reagent. This reagent consists of acetylthiocholine and 5,5'-dithio-bis-(2-nitrobenzoic acid). Hydrolysis of acetylthiocholine by AChE produces thiocholine (see Figure). The non-enzymatic reaction of thiocholine with 5,5'-dithio-bis-(2-nitrobenzoic acid) produces 5-thio-2-nitrobenzoic acid, which has a strong absorbance at 412 nm ( $\epsilon = 13,600$ ).

AChE has several advantages over other enzymes commonly used for enzyme immunoassays. Unlike

horseradish peroxidase, AChE does not self-inactivate during turnover. This property of AChE also allows redevelopment of the assay if it is accidentally splashed or spilled. In addition, the enzyme is highly stable under the assay conditions, has a wide pH range (pH 5-10), and is not inhibited by common buffer salts or preservatives. Since AChE is stable during the development step, it is unnecessary to use a 'stop' reagent, and the plate may be read whenever it is convenient.

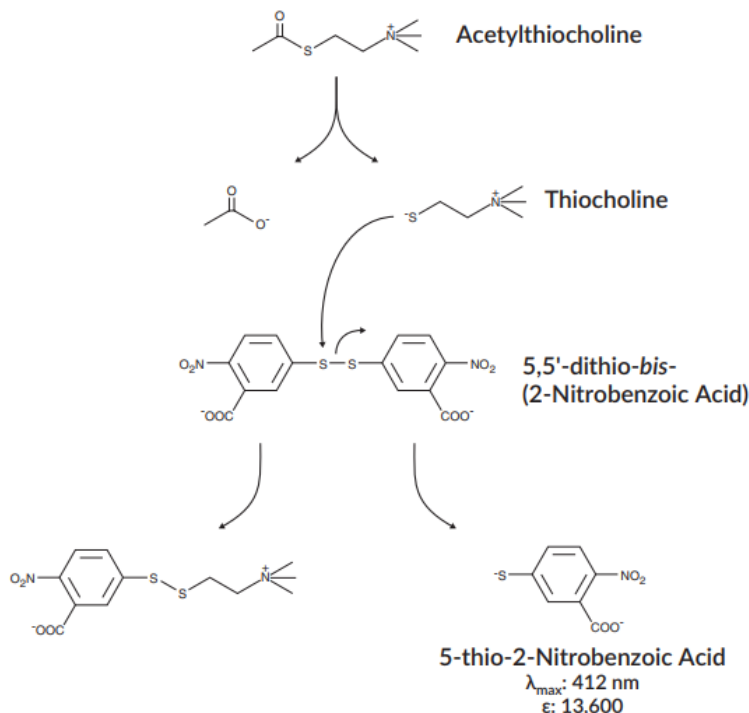

**Figure: Reaction catalyzed by acetylcholinesterase**

## Reagents And Materials Provided

1. Cyclic AMP ELISA Anti serum, 1vial/100 dtn, -20°C
2. Cyclic AMP AChE Tracer, 1vial/100 dtn, -20°C
3. Cyclic AMP ELISA Standard, 1 vial, -20°C
4. ELISA Buffer Concentrate(10×), 2vials/10 ml, -20°C
5. Wash Buffer Concentrate(400×), 1 vial/5 ml, -20°C
6. Polysorbate 20, 1 vial/3 ml, -20°C
7. Mouse Anti-Rabbit IgG Coated Plate, 1 plate, -20°C
8. 96-Well Cover Sheet, 1cover, -20°C
9. Ellman's Reagent, 3 vials/100 dtn, -20°C
10. Acetic Anhydride, 1 vial/2.5 ml, -20°C
11. Potassium Hydroxide, 1 vial, -20°C
12. ELISA Tracer Dye, 1vial, -20°C
13. ELISA Antiserum Dye, 1 vial, -20°C

## Materials Required But Not Supplied

1. A plate reader capable of measuring absorbance between 405-420 nm.
2. Adjustable pipettes and a repeating pipettor.
3. A source of 'UltraPure' water. Water used to prepare all ELISA reagents and buffers must be deionized and free of trace organic contaminants (UltraPure®). Use activated carbon filter cartridges or other organic scavengers. Glass distilled water (even if double distilled), HPLC-grade water, and sterile water (for injections) are not adequate for ELISA.
4. Materials used for Specimen Collection And Preparation.

## Storage

This kit will perform as specified if stored as directed at -20°C and used before the expiration date indicated on the outside of the box.

## Specimen Collection And Preparation

In general, urine and tissue culture supernatant samples may be diluted with ELISA Buffer and added directly to the assay well. Plasma, serum, whole blood, and tissue homogenates, as well as other heterogeneous mixtures such as lavage fluids and aspirates often contain contaminants which can interfere in the assay. The presence of rabbit IgG in the sample may cause interference in the assay. It is best to check for interference before embarking on a large number of

sample measurements. To test for interference, dilute one or two test samples to obtain at least two different dilutions of each sample between ~20-80% B/B<sub>0</sub> on the standard curve. If the two different dilutions of the sample show good correlation (differ by 20% or less) in the final calculated cAMP concentration, purification is not required. If you do not see good correlation of the different dilutions, purification is advised. Due to the presence of phosphodiesterases

in many samples (i.e., tissues and cell lysates), sample purification is mandatory to prevent enzymatic hydrolysis of cAMP. Protocols for sample preparation are provided below:

### General Precautions

All samples must be free of organic solvents prior to assay.

Samples should be assayed immediately after collection; samples that cannot be assayed immediately should be stored at -80°C.

Samples of rabbit origin may contain antibodies which interfere with the assay by binding to the mouse anti-rabbit plate. We recommend that all rabbit samples be purified prior to use in this assay.

### Urine

Urine samples may be diluted in ELISA Buffer and assayed directly. Dilutions of between approximately 1:200 and 1:500 may be required for measurement of cAMP in urine.

### Plasma

To 500 µl plasma add 2 ml ice cold ethanol and vortex. Leave the sample at room temperature for five minutes. Remove the precipitate by centrifugation at 1,500 x g for 10 minutes and transfer the supernatant to

a clean 10 ml test tube. Dry the supernatant by vacuum centrifugation or under a stream of nitrogen and then resuspend in 500 µl of ELISA Buffer (vacuum centrifugation can be used to remove the final aqueous portion of the extract). Ensure that all of the ethanol is removed as trace amounts can affect the performance of the assay.

### Culture Medium Samples

Cell culture supernatants may be assayed directly without purification. If the cAMP concentration in the medium is high enough to dilute the sample 10-fold with ELISA Buffer, the assay can be performed without any modifications. When assaying less concentrated samples (where samples cannot be diluted with ELISA Buffer), dilute the standard curve in the same culture medium as that used in the experiment. This will ensure that the matrix for the standards is comparable to the samples. We recommend that a standard curve be run first to ensure that the assay will perform in a particular medium.

### Cell Culture Extraction for cAMP Assay

- a. Aspirate medium from plate/flask.
- b. Add 1 ml of 0.1 M HCl for every 35 cm<sup>2</sup> of surface area (e.g., for a 150 mm plate, add 5 ml).
- c. Incubate at room temperature for 20 minutes.
- d. Scrape cells off the surface with a cell scraper or rubber policeman.
- e. Dissociate the mixture by pipetting up and down until the suspension is homogeneous, and transfer to appropriately sized centrifuge tube.
- f. Centrifuge at 1,000 x g for 10 minutes.
- g. Decant the supernatant into a clean test tube.

Dilute the supernatants at least 1:2 in ELISA buffer to neutralize the acid prior to performing the assay. A protein concentration of at least 1 mg/ml in the supernatant is recommended for reproducible results.

If acetylation is required, follow the procedure for sample acetylation in Assay Procedure.

### Tissue Samples

- a. Cyclic nucleotides may be metabolized quickly in tissue, so it is important to rapidly freeze (i.e., using liquid nitrogen) the sample immediately after collection.
- b. Weigh the frozen tissue and drop into 5-10 volumes (ml of solution/gram of tissue) of 5% trichloroacetic acid (TCA) in water. Homogenize the sample on ice (0-4°C) using a Polytron-type homogenizer. **NOTE:** Alternatively the frozen sample can be pulverized prior to addition of TCA.
- c. Remove the precipitate by centrifugation at 1,500 x g for 10 minutes. Carefully transfer the supernatant to a clean test tube.
- d. Extract the TCA from the sample using water-saturated ether. **NOTE:** To make water-saturated ether, add water to ether until layers form; mix and use the top (ether) layer. Add five volumes of ether to one volume of supernatant, mix for 10 seconds, and then allow the organic and aqueous phases to separate. Carefully remove the top ether layer and discard. Repeat the extraction two more times.
- e. Remove the residual ether from the aqueous layer by heating the sample to 70°C for five minutes. It is imperative that all the ether be removed as even trace amounts can interfere with the assay.

Supernatants from the tissue extraction can be assayed directly without dilution provided the standard curve is prepared in the same matrix as the samples. To prepare the standard curve matrix solution, extract about 20 ml of the 5% TCA preparation with ether in the same manner as used for sample extraction. Remove the

residual ether by heating and use the remaining solution to prepare the standard curve.

## Plate Preparation

The 96-well plate(s) included with this kit is supplied ready to use. It is not necessary to rinse the plate(s) prior to adding the reagents. **NOTE:** If you do not need to use all the strips at once, place the unused strips back in the plate packet and store at 4°C. Be sure the packet is sealed with the desiccant inside.

Each plate or set of strips must contain a minimum of two blanks (Blk), two non-specific binding wells (NSB), two maximum binding wells ( $B_0$ ), and an eight point standard curve run in duplicate. **NOTE:** Each assay must contain this minimum configuration in order to ensure accurate and reproducible results. Each sample should be assayed at two dilutions and each dilution should be assayed in duplicate. For statistical purposes, we recommend assaying samples in triplicate.

A suggested plate format is shown in Figure 5, below. We suggest you record the contents of each well on the sheet.

	1	2	3	4	5	6	7	8	9	10	11	12
A	Blk	S1	S1	1	1	1	9	9	9	17	17	17
B	Blk	S2	S2	2	2	2	10	10	10	18	18	18
C	NSB	S3	S3	3	3	3	11	11	11	19	19	19
D	NSB	S4	S4	4	4	4	12	12	12	20	20	20
E	$B_0$	S5	S5	5	5	5	13	13	13	21	21	21
F	$B_0$	S6	S6	6	6	6	14	14	14	22	22	22
G	$B_0$	S7	S7	7	7	7	15	15	15	23	23	23
H	TA	S8	S8	8	8	8	16	16	16	24	24	24

Blk - Blank  
 TA - Total Activity  
 NSB - Non-Specific Binding  
 $B_0$  - Maximum Binding  
 S1-S8 - Standards 1-8  
 1-24 - Samples

**Figure: Sample plate format**

## Reagent Preparation

**NOTE:** Water used to prepare all ELISA reagents and buffers must be deionized and free of trace organic contaminants (UltraPure®). Use activated carbon filter cartridges or other organic scavengers. Glass distilled water (even if double distilled), HPLC-grade water, and sterile water (for injections) are not adequate for ELISA.

Store all diluted buffers at 4°C; they will be stable for about two months.

### 1. ELISA Buffer Preparation

Dilute the contents of one vial of ELISA Buffer Concentrate (10x) with 90 ml of UltraPure water. Be certain to rinse the vial to remove any salts that may have precipitated. **NOTE: It is normal for the concentrated buffer to contain crystalline salts after thawing. These will completely dissolve upon dilution with water.**

### 2. Wash Buffer Preparation

5 ml vial Wash Buffer Concentrate (400x) (96-well kit): Dilute to a total volume of 2 liters with UltraPure water and add 1ml of Polysorbate 20.

Smaller volumes of Wash Buffer can be prepared by diluting the Wash Buffer Concentrate 1:400 and adding Polysorbate 20 (0.5 ml/liter of Wash Buffer).

**NOTE: Polysorbate 20 is a viscous liquid and cannot be measured by a regular pipette. A positive displacement pipette or a syringe should be used to deliver small quantities accurately.**

### 3. cAMP AChE Tracer

Reconstitute the cAMP AChE Tracer as follows:

100 dtn cAMP AChE Tracer (96-well kit): Reconstitute with 6 ml ELISA Buffer.

Store the reconstituted cAMP AChE Tracer at 4°C (do not freeze!) and use within four weeks. A 20% surplus of tracer has been included to account for any incidental losses.

**Tracer Dye Instructions (optional):** This dye may be added to the tracer, if desired, to aid in visualization of tracer-containing wells. Add the dye to the reconstituted tracer at a final dilution of 1:100 (add 60 µl of dye to 6 ml tracer or add 300 µl of dye to 30 ml of tracer).

### 4. cAMP ELISA Antiserum

Reconstitute the cAMP ELISA Antiserum as follows:

100 dtn cAMP ELISA Antiserum: Reconstitute with 6 ml ELISA Buffer.

Store the reconstituted cAMP ELISA Antiserum at 4°C. It will be stable for at least four weeks. A 20% surplus of antiserum has been included to account for any incidental losses.

**Antiserum Dye Instructions (optional):** This dye may be added to the antiserum, if desired, to aid in visualization of antiserum-containing wells. Add the dye to the reconstituted antiserum at a final dilution of 1:100 (add 60 µl of dye to 6 ml antiserum or add 300 µl of dye to 30 ml of antiserum).

### 5. cAMP Standards and Samples

Do you need to acetylate?

The ELISA is able to detect lower concentrations of cAMP if the samples are first acetylated. If the expected cAMP concentration is less than 5 pmol/ml, the acetylation procedure should be performed. If the expected concentration is greater than 5 pmol/ml no acetylation is necessary. **NOTE:** The acetylation procedure may be affected by proteins or sugars in the sample matrix. In these cases, the sample should be purified before acetylation.


#### 1) Preparation of Standards and Samples - No Acetylation

##### a. Standard Curve Preparation

Reconstitute the cAMP ELISA Standard with 1 ml of ELISA Buffer. The concentration of this solution will be 7,500 pmol/ml. Store this solution at 4°C; it will be stable for approximately six weeks. We have included enough cAMP to run ten standard curves. This surplus should accommodate any experimental design.

**NOTE:** If the samples are prepared from TCA-extracted tissue and cannot be diluted at least 1:5 in ELISA Buffer for analysis, use ether-extracted 5% TCA for preparation of the standard curve. Any dilution of samples should also be performed in 5%TCA.

To prepare the standard for use in ELISA: Obtain eight clean test tubes and number them #1 through #8. Aliquot 900 µl ELISA Buffer to tube #1 and 600 µl ELISA Buffer to tubes #2-8. Transfer 100 µl of the bulk standard (7,500 pmol/ml) to tube #1 and mix thoroughly. The concentration of this standard, the first point on the standard curve, is 750 pmol/ml. Serially dilute the standard by removing 300 µl from tube #1 and placing in tube #2; mix thoroughly. Next, remove 300 µl from tube #2 and place it into tube #3; mix thoroughly. Repeat this process for tubes #4-8. These diluted standards should not be stored for more than 24 hours.

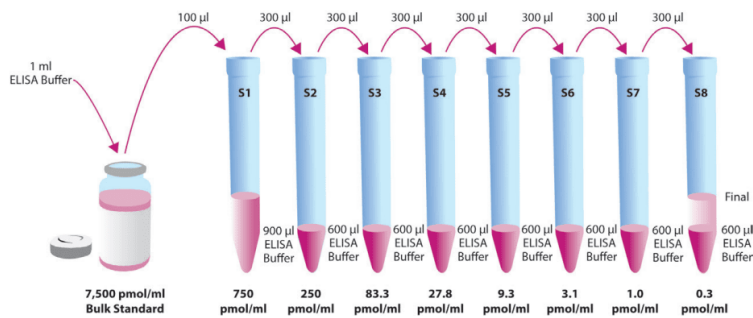

**Figure: Preparation of non-acetylated cAMP standards**

## b. Sample preparation

If samples require purification, please refer to the protocols in Specimen Collection And Preparation.

Upon purification, no further sample preparation is necessary; however, the samples may require dilution to ensure that they will fall on the linear portion of the standard curve (20-80% B/B<sub>0</sub>). Proceed to Assay Procedure.


## 2) Preparation of Standards and Samples - Acetylation

### a. Standard Curve Preparation

Reconstitute the cAMP ELISA Standard (Item No. 481004) with 1 ml of ELISA Buffer (label this Standard A). Aliquot 80 µl of Standard A (7,500 pmol/ml) into 2.920 ml of ELISA Buffer (label this Standard B). The concentration of this standard is 200 pmol/ml.

**NOTE:** If the samples are prepared from TCA-extracted tissue and cannot be diluted at least 1:5 in ELISA Buffer for analysis, use ether-extracted 5% TCA for preparation of the standard curve. Any dilution of samples should also be performed in this 5% TCA.

To prepare the standard for use in ELISA: Obtain nine clean test tubes and number them #0 through #8. Aliquot 500 µl ELISA Buffer to tube #0 (this tube will contain only buffer), 950 µl ELISA Buffer to tube #1 and 500 µl ELISA Buffer to tubes #2-8. Transfer 50 µl of Standard B (200 pmol/ml) to tube #1; mix thoroughly. The concentration of this standard, the first point on the standard curve, is 10 pmol/ml. Serially dilute the standard by removing 500 µl from tube #1 and placing in tube #2; mix thoroughly. Next, remove 500 µl from tube #2 and place it into tube #3; mix thoroughly. Repeat this process for tubes #4-8. Discard 500 µl of the solution in tube #8 so each tube contains 500 µl. These diluted standards should not be stored for more than 24 hours.

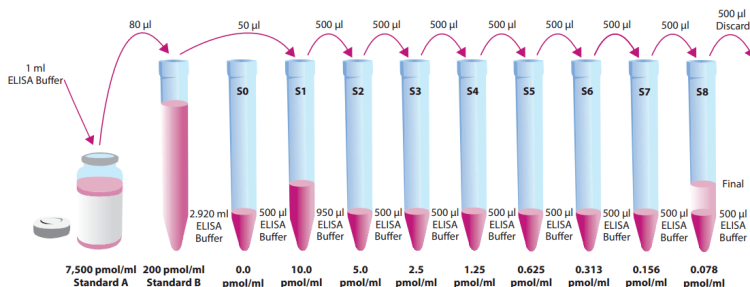

**Figure: Preparation of acetylated cAMP standards**

## b. Sample preparation

If samples need to be purified, do so before proceeding with the acetylation procedure (see page 12-15 for Purification Protocol). Although purification may not be necessary, we recommend that samples be purified to



ensure assay integrity. If you are acetylating less than 500 µl of sample, you must adjust the amounts of Potassium Hydroxide (KOH) and acetic anhydride proportionally.

### Preparation of KOH

Prepare a 4 M solution of KOH: 100 dtn Potassium Hydroxide (96-well kit): Dissolve with 10 ml UltraPure water.

### Acetylation procedure(based on 500 µl sample size)

All samples, as well as standard tubes #O-8, must be acetylated. Each sample/standard should be acetylated individually. It is important to be consistent in the acetylation technique as differences in vortex time and/or delayed addition of KOH may result in irreproducible results.

To 500 µl of sample, add 100 µl of 4 M KOH and 25 µl Acetic Anhydride in quick succession. Vortex for 15 seconds. Add 25 µl of 4 M KOH and vortex.

Repeat for all samples and standard tubes.

**NOTE:** If the samples contain sugars at concentration >250 mM, it may be necessary to proportionately increase the amount of KOH and acetic anhydride added to ensure complete acetylation of cAMP.

## Assay Procedure

### Pipetting Hints

Use different tips to pipette each reagent.

Before pipetting each reagent, equilibrate the pipette tip in that reagent(i.e., slowly fill the tip and gently expel the contents, repeat several times).

Do not expose the pipette tip to the reagent(s) already in the well.

### Addition of the Reagents

#### 1. ELISA Buffer

Add 100 µl ELISA Buffer to NSB wells. Add 50 µl ELISA Buffer to B<sub>0</sub> wells. If culture medium or ether-saturated 5% TCA was used to dilute the standard curve, substitute 50 µl of that matrix for ELISA Buffer in the NSB and B<sub>0</sub> wells (i.e., add 50 µl culture medium to NSB and B<sub>0</sub> wells and 50 µl ELISA Buffer to NSB wells). If standards and samples were acetylated, substitute 50 µl of acetylated sample matrix(tube #0) for ELISA Buffer in the NSB and B<sub>0</sub> wells (i.e., add 50 µl of tube #O to NSB and B<sub>0</sub> wells and 50 µl of ELISA Buffer to NSB wells).

#### 2. cAMP ELISA Standard

Add 50 µl from tube # 8 to both of the lowest standard wells (S8). Add 50 µl from tube # 7 to each of the next two standard wells (S7). Continue with this procedure until all the standards are aliquoted. The same pipette tip should be used to aliquot all the standards. Before pipetting each standard, be sure to equilibrate the pipette tip in that standard.

#### 3. Samples

Add 50 µl of sample per well. Each sample should be assayed at a minimum of two dilutions. Each dilution should be assayed in duplicate (triplicate recommended),

#### 4. cAMP AChE Tracer

Add 50 µl to each well except the TA and the Blk wells.

## 5. cAMP ELISA Antiserum

Add 50 µl to each well except the TA, the NSB, and the Blk wells.

Well	ELISA Buffer	Standard/Sample	Tracer	Antiserum
Blk	-	-	-	-
TA	-	-	5 µl (at devl. step)	-
NSB	100 µl	-	50 µl	-
B <sub>0</sub>	50 µl	-	50 µl	50 µl
Std/Sample	-	50 µl	50 µl	50 µl

Table 1. Pipetting summary

## Incubation of the Plate

Cover each plate with plastic film and incubate 18 hours at 4°C.

## Development of the Plate

1. Reconstitute Ellman's Reagent immediately before use (20 ml of reagent is sufficient to develop 100 wells): 100 dtn vial Ellman's Reagent (96-well kit): Reconstitute with 20 ml of UltraPure water.  
**NOTE:** Reconstituted Ellman's Reagent is unstable and should be used the same day it is prepared; protect the Ellman's Reagent from light when not in use. Extra vials of the reagent have been provided should a plate need to be re-developed or multiple assays be run on different days.
2. Empty the wells and rinse five times with Wash Buffer.
3. Add 200 µl of Ellman's Reagent to each well.
4. Add 5 µl of tracer to the TA wells.
5. Cover the plate with plastic film. Optimum development is obtained by using an orbital shaker equipped with a large, flat cover to allow the plate(s) to develop in the dark. This assay typically develops (i.e., B<sub>0</sub> wells  $\geq 0.3$  A.U. (blank subtracted)) in 90-120 minutes.

## Reading the Plate

1. Wipe the bottom of the plate with a clean tissue to remove fingerprints, dirt, etc.
2. Remove the plate cover being careful to keep Ellman's Reagent from splashing on the cover. **NOTE:** Any loss of Ellman's Reagent will affect the absorbance readings. If Ellman's Reagent is present on the cover, use a pipette to transfer the Ellman's Reagent into the well. If too much Ellman's Reagent has splashed on the cover to easily redistribute back into the wells, wash the plate three times with wash buffer and repeat the development with fresh Ellman's Reagent.
3. Read the plate at a wavelength between 405 and 420 nm. The absorbance may be checked periodically until the B<sub>0</sub> wells have reached a minimum of 0.3 A.U. (blank subtracted). The plate should be read when the absorbance of the B<sub>0</sub> wells are in the range of 0.3-1.0 A.U. (blank subtracted). If the absorbance of the wells exceeds 1.5, wash the plate, add fresh Ellman's Reagent and let it develop again.

## Calculation

Many plate readers come with data reduction software that plot data automatically. Alternatively a spreadsheet program can be used. The data should be plotted as either %B/B<sub>0</sub> versus log concentration using a four-parameter logistic fit or as logit B/B<sub>0</sub> versus log concentration using a linear fit.

## Calculations

### 1. Preparation of the Data

The following procedure is recommended for preparation of the data prior to graphical analysis.

**NOTE:** If the plate reader has not subtracted the absorbance readings of the blank wells from the absorbance readings of the rest of the plate, be sure to do that now.

- a. Average the absorbance readings from the NSB wells.
- b. Average the absorbance readings from the B<sub>0</sub> wells.
- c. Subtract the NSB average from the B<sub>0</sub> average. This is the corrected B<sub>0</sub> or corrected maximum binding.
- d. Calculate the B/B<sub>0</sub> (Sample or Standard Bound/Maximum Bound) for the remaining wells. To do this, subtract the average NSB absorbance from the S1 absorbance and divide by the corrected B<sub>0</sub> (from Step 3). Repeat for S2-S8 and all sample wells. (To obtain %B/B<sub>0</sub> for a logistic four-parameter fit, multiply these values by 100.)

**NOTE:** The TA values are not used in the standard curve calculations. Rather, they are used as a diagnostic tool; the corrected B<sub>0</sub> divided by the actual TA (10x measured absorbance) will give the %Bound. This value should closely approximate the %Bound that can be calculated from the Sample Data. Erratic absorbance values and a low (or no) %Bound could indicate the presence of organic solvents in the buffer or other technical problems.

### 2. Plot the Standard Curve

Plot %B/B<sub>0</sub> for standards S1-S8 versus cAMP concentration using linear (y) and log (x) axes and perform a 4-parameter logistic fit.

Alternative Plot - The data can also be linearized using a logit transformation. The equation for this conversion is shown below. **NOTE: Do not use %B/B<sub>0</sub> in this calculation.**

$$\text{logit} (B/B_0) = \ln [B/B_0 / (1 - B/B_0)]$$

Plot the data as logit (B/B<sub>0</sub>) versus log concentrations and perform a linear regression fit.

### 3. Determine the Sample Concentration

Calculate the B/B<sub>0</sub> (or %B/B<sub>0</sub>) value for each sample. Determine the concentration of each sample using the equation obtained from the standard curve plot. **NOTE:** Remember to account for any concentration or dilution of the sample prior to the addition to the well. Samples with %B/B<sub>0</sub> values greater than 80% or less than 20% should be re-assayed as they generally fall out of the linear range of the standard curve. A 20% or greater disparity between the apparent concentration of two different dilutions of the same sample indicates interference which could be eliminated by purification.


## Typical Standard Curve

The standard curves presented here are examples of the data typically produced with this kit; however, your results will not be identical to these. You must run a new standard curve. Do not use the data below to determine the values of your samples. Your results could differ substantially.

**Sample Data (Non-Acetylated)**

	Raw Data		Average	Corrected
Total Activity	3.312	3.308	3.310	3.308
NSB	-0.003	-0.001	-0.002	
B <sub>0</sub>	0.956	0.972		
	0.960	1.011	0.975	0.977

Dose (pmol/ml)	Raw Data		Corrected		%B/B <sub>0</sub>	
750	0.053	0.054	0.055	0.056	5.7	5.7
250	0.148	0.135	0.150	0.137	15.4	14.1
83.3	0.256	0.255	0.258	0.257	26.5	26.4
27.8	0.435	0.436	0.437	0.438	44.8	45.0
9.3	0.621	0.632	0.623	0.634	63.9	65.1
3.1	0.792	0.801	0.794	0.803	81.4	82.4
1.0	0.888	0.887	0.890	0.889	91.3	91.2
0.3	0.927	0.913	0.929	0.915	95.3	93.9

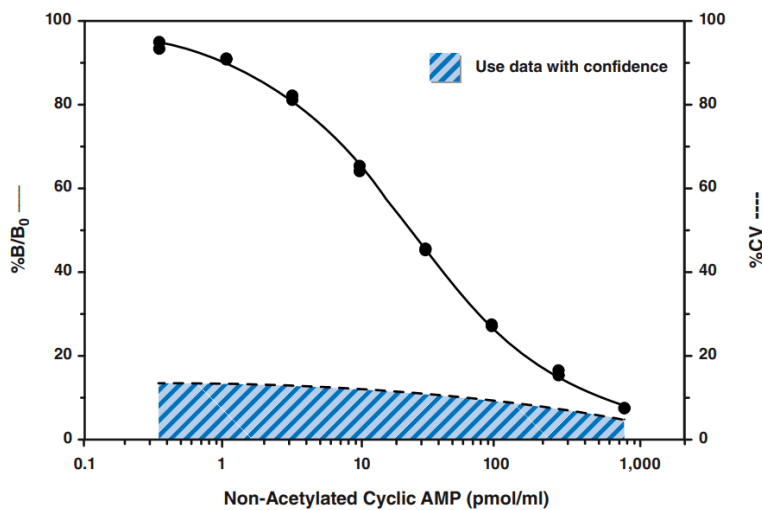**Table. Typical results for non-acetylated cAMP**

Assay Range = 0.3-750 pmol/ml

Sensitivity (defined as 80% B/B<sub>0</sub>) = 3 pmol/ml

Mid-point(defined as 50% B/B<sub>0</sub>)= 15-25 pmol/ml


The sensitivity and mid-point were derived from the standard curve shown above. The standard was diluted with ELISA Buffer.

**Sample Data (Acetylated)**

	Raw Data		Average	Corrected
Total Activity	3.903	3.883	3.863	
NSB	-0.002	0.001	-0.001	
B <sub>0</sub>	0.611	0.651		
	0.586	0.585	0.608	0.609

Dose (pmol/ml)	Raw Data		Corrected		%B/B <sub>0</sub>	
10.0	0.059	0.055	0.060	0.056	9.7	9.2
5.0	0.080	0.091	0.081	0.092	13.3	15.0
2.5	0.116	0.125	0.117	0.126	91.2	20.6
1.25	0.179	0.179	0.180	0.180	29.6	29.5
0.625	0.258	0.277	0.259	0.278	42.5	45.7
0.313	0.345	0.361	0.346	0.362	56.9	59.5
0.156	0.447	0.429	0.448	0.430	73.6	70.7
0.078	0.517	0.510	0.518	0.511	85.1	83.9

**Table. Typical results for acetylated cAMP**

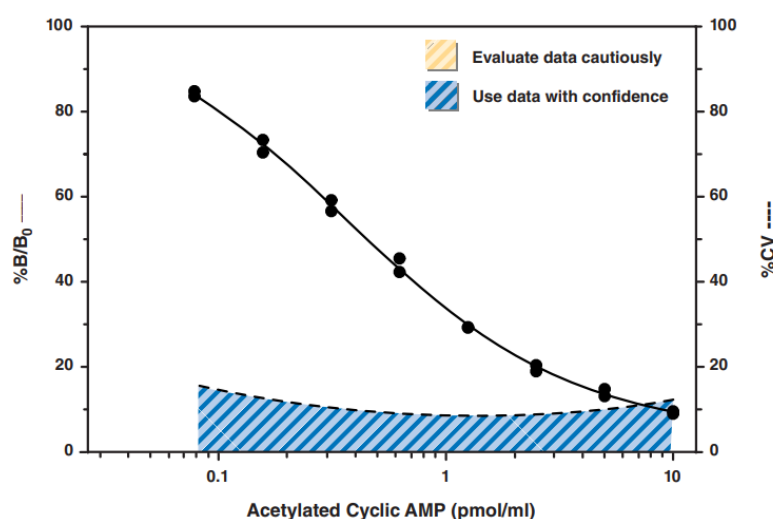

Assay Range = 0.078-10 pmol/ml

Sensitivity(defined as 80% B/Bo)= 0.1 pmol/ml

Mid-point (defined as 50% B/Bo)= 0.5 pmol/ml

The sensitivity and mid-point were derived from the standard curve shown above. The standard was diluted with ELISA Buffer.

## Precision

### Non-Acetylated

The intra- and inter-assay CVs have been determined at multiple points on the standard curve.

Dose (pmol/ml)	%CV* Intra-assay variation	%CV* Inter-assay variation
750	6.7	6.3
250	7.3	5.3
83.3	7.6	8.3
27.8	10.9	5.4
9.3	12.1	16.0
3.1	18.5	15.2
1.0	12.9	23.0
0.3	11.6	20.3

**Table. Intra- and inter-assay variation of the non-acetylated cAMP assay.** \*%CV represents the variation in concentration (not absorbance) as determined using a reference standard curve.

### Acetylated

The intra- and inter-assay CVs have been determined at multiple points on the standard curve.

Dose (pmol/ml)	%CV* Intra-assay variation	%CV* Inter-assay variation
10.0	11.5	8.1
5.0	12.1	7.1
2.5	8.6	10.0
1.25	8.7	12.8
0.625	8.7	4.1
0.313	11.4	9.2
0.156	11.0	12.4
0.078	17.0	8.2

**Table. Intra- and inter-assay variation of the acetylated cAMP assay.**

\*%CV represents the variation in concentration (not absorbance) as determined using a reference standard curve.

### Specificity

Non-Acetylated		Acetylated	
Compound	Cross Reactivity	Compound	Cross Reactivity
cAMP	100%	Acetylated cAMP	100%
cGMP	1.5%	Acetylated cGMP	0.69%
Adenosine	<0.01%	Acetylated Adenosine	<0.01%
AMP	<0.01%	Acetylated AMP	<0.01%
ATP	<0.01%		

## Precautions

Please read these instructions carefully before beginning this assay.

The reagents in this kit have been tested and formulated to work exclusively with the Cyclic AMP ELISA Kit. This kit may not perform as described if any reagent or procedure is replaced or modified. When compared to quantification by LC/MS or GC/MS, it is not uncommon for immunoassays to report higher analyte concentrations. While LC/MS or GC/MS analyses typically measure only a single compound, antibodies used in immunoassays sometimes recognize not only the target molecule, but also structurally related molecules, including biologically relevant metabolites. In many cases, measurement of both the parent molecule and metabolites is more representative of the overall biological response than is the measurement of a short-lived parent molecule. It is the responsibility of the researcher to understand the limits of both assay systems and to interpret their data accordingly.