



User's Manual

Porcine CTXI(Cross Linked C-telopeptide of Type I Collagen) ELISA Kit

REF

DEIA-NS2307-98



96T

RUO

This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

Creative Diagnostics

 Address: 45-1 Ramsey Road, Shirley, NY 11967, USA

 Tel: 1-631-624-4882 (USA) 44-161-818-6441 (Europe)  Fax: 1-631-938-8221

 Email: info@creative-diagnostics.com  Web: www.creative-diagnostics.com

PRODUCT INFORMATION


Intended Use

In vitro quantitative determination of CTXI concentrations in serum, plasma, cell culture supernatant and other biological samples.

Storage

2-8 °C for 6 months

Typical Standard Curve

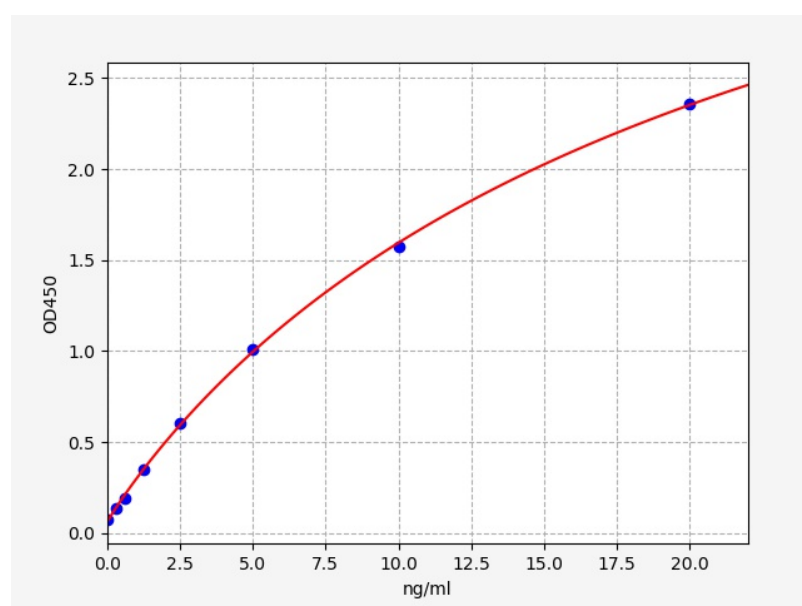

Performance Characteristics

Perform the stability test for the sealed kit at 37°C and 2-8°C and get relevant data.

Elisa kit(n=5)	37°C for 1 month	2-8°C for 6 months
Average (%)	80	95-100

Precision

Intra-Assay: CV<8%

Inter-Assay: CV<10%

Detection Range

0.313-20ng/ml

Sensitivity

< 0.188ng/ml

Specificity

Specifically recognize CTXI, no obvious cross reaction with other analogues

Linearity

Dilute the sample with a certain amount of CTXI at 1:2, 1:4 and 1:8 to get the recovery range.

Sample	1:2	1:4	1:8
Serum(n=5)	89-103%	87-102%	86-93%
EDTA Plasma(n=5)	82-99%	88-96%	83-101%
Heparin Plasma(n=5)	86-98%	83-99%	87-100%

Recovery

Add a certain amount of CTXI into the sample. Calculate the recovery by comparing the measured value with the expected amount of CTXI in the sample.

Matrix	Recovery Range (%)	Average (%)
Serum(n=5)	89-98	94
EDTA Plasma(n=5)	86-103	97
Heparin Plasma(n=5)	86-102	93