



User's Manual

Benzonase Nuclease ELISA Kit

REF

DEIA-PX0001



96T

RUO

This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

Creative Diagnostics

 **Address: 45-1 Ramsey Road, Shirley, NY 11967, USA**

 **Tel: 1-631-624-4882 (USA) 44-161-818-6441 (Europe)**  **Fax: 1-631-938-8221**

 **Email: info@creative-diagnostics.com**  **Web: www.creative-diagnostics.com**

PRODUCT INFORMATION

Intended Use

The Benzonase Nuclease ELISA Detection Kit is designed for the quantitative detection of residual nuclease content in intermediates, semi-finished products and finished products of various biological products.

Principles of Testing

The kit can quantitative detect trace residual Benzonase nuclease (hereinafter referred to as "nuclease") in test samples by using a double-antibody sandwich method. Coat the 96-well plate with capture antibody to prepare immobilized antibodies.

Add the standard and test samples, and then horseradish peroxidase (HRP) conjugated antibody to form an immobilized antibody-nuclease-conjugated antibody sandwich conjugate. Wash the plate after reaction, and add the substrate for color development reaction. The substrate will turn blue under HRP catalysis, and will finally turn yellow under the action of the stop solution. Determine the optical density (OD) value at 450 nm, and calculate the nuclease content in the test sample using the standard curve.

Reagents And Materials Provided

1. Benzonase Coated Plate, 8 wells × 12 strips, Ready-to-use
2. Benzonase Standard (standard), 100 µL × 1 vial (0.5 µg/mL), Operate as per the recommended dilution procedure
3. Anti-Benzonase (enzyme-labeled antibody), 15 mL × 1 bottle, Ready-to-use
4. Sample Diluent Buffer, 30 mL × 1 bottle, Ready-to-use
5. 20× Wash Buffer, 30 mL × 1 bottle, Operate as per the recommended dilution procedure
6. Color Reagent A, 8 mL × 1 vial, Ready-to-use
7. Color Reagent B, 8 mL × 1 vial, Ready-to-use
8. Stop Solution, 15 mL × 1 bottle, Ready-to-use
9. Plate Sealer, 3 pieces, Ready-to-use
10. Instructions for Use, 1 copy

Notes: Reagents should be stored at 2 ~ 8°C; Color Reagents A and B should be protected from light during storage.

Materials Required But Not Supplied

1. Plate reader, thermostate plate shaker or thermostate incubator, plate washer
2. High-precision pipette and disposable tips (0.5 ~ 10 µL, 10 ~ 100 µL, 30 ~ 300 µL, and 100 ~ 1000 µL).
3. Deionized water, blotting paper, EP tubes

Storage


The shelf life of unopened kits is 12 months when stored at 2 ~ 8°C.

Reagent Preparation

1. 1× Wash Buffer: Take 1 portion of Wash Buffer (20×), and add 19 times the volume of deionized water to prepare the Wash Buffer at working concentration (1×). If there are crystals in the Wash Buffer (20×), shake gently at room temperature or in a 37°C water bath, and dilute after the crystals are completely dissolved. Unused Wash Buffer (20×) should be stored at 2 ~ 8°C.
2. Preparation of standard: Dilute the standard to 5 ng/mL with the Sample Diluent Buffer, and prepare the standard by 2.5-fold dilution.
3. Preparation of substrate solution: Mix Color Reagents A and B at equal volume at 10 minutes before use, and the operation should be performed at dark environment. Make sure that the substrate solution is not contaminated. Do not use if the substrate solution turns blue after mixing.

Assay Procedure

1. Equilibrate the temperature of each component in the kit to room temperature for 30 minutes. Take out required strip plates from aluminum foil bags already equilibrated to room temperature, and label the strip plate sequence with a marker. Seal remaining strip plates with a plate sealer, put them back to the aluminum foil bag, then seal the bag, and store at 2 ~ 8°C.
2. Preparation of standard: Dilute the standard to 5 ng/mL with the Sample Diluent Buffer, and prepare the standard by 2.5-fold dilution, as shown in the figure on the right.

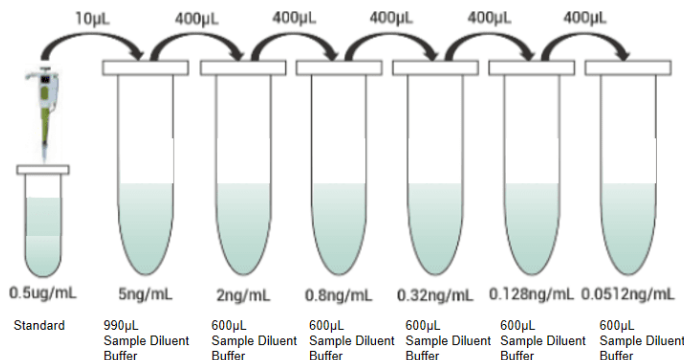


3. Sample incubation: Set the standard wells, blank wells, and test sample wells, respectively. Add standards at different concentrations (in sequence), Sample Diluent Buffer, and test sample to standard wells, blank wells, and test sample wells, respectively (100 µL/well), seal the plate with a plate sealer, and incubate at 37°C for 1 hour.
4. Plate washing: Discard liquid in the wells. Wash the plate for 3 times with 1× Wash Buffer (250 µL/well), and pat dry the residual liquid in test sample wells. (After adding the Wash Buffer each time, if the plate is to be washed manually, allow the plate to stand for 1 minute after adding the Wash Buffer and shake gently; if the plate is to be washed with a plate washer, shake the plate gently for 5 seconds after adding the Wash Buffer.)
5. Incubation of enzyme-labeled antibody: Add 100 µL of enzyme-labeled antibody into each well, seal the plate with a plate sealer, and incubate at 37°C for 1 hour.
6. Plate washing: Same as Step 4.

7. Color development: Add the pre-prepared substrate solution into the plate (100 μ L/well) and mix well, seal the plate with a plate sealer, and incubate at 37°C for 15 minutes while being protected from light.
8. Reaction termination: Add stop solution at 100 μ L/well.
9. Reading: Measure the OD values at 450 nm and 630 nm with a plate reader. The measurement should be completed within 20 minutes after reaction termination.

Calculation

Plot the curve with the OD value (OD_{450 nm} - OD_{630 nm}) of the nuclease standard as the dependent variable Y and the standard concentration as the independent variable X. The 4-parameter logistic fitting equation is recommended: $Y = ((A - D)/(1 + (x/C)^B) + D$. Substitute the OD value of test sample (OD_{450 nm} - OD_{630 nm}) to the equation to calculate the nuclease content in the test sample).

Typical Standard Curve

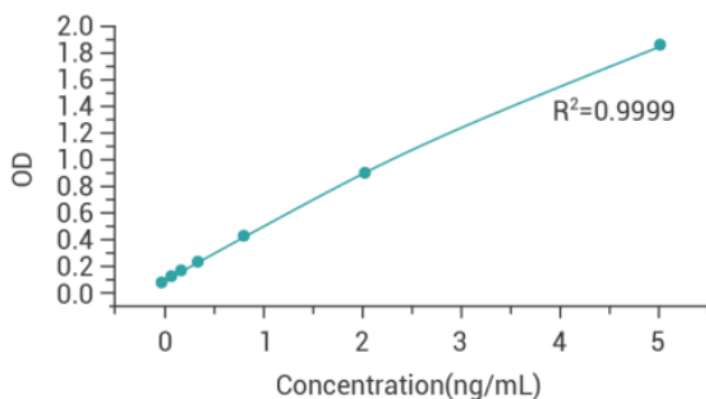

Standard concentration (ng/mL)	OD value (1)	OD value (2)	Mean value
5	1.925	1.774	1.849
2	0.917	0.865	0.891
0.8	0.447	0.441	0.444
0.32	0.228	0.209	0.218
0.128	0.146	0.137	0.141
0.0512	0.114	0.107	0.110

Precautions

1. This kit is for in vitro detection only, and may not be used for clinical diagnosis.
2. The kit must be used within the shelf life.
3. All components in the kit must be equilibrated to room temperature (20 ~ 25°C) before use.
4. Fully mix each components of the kit before use. When patting to dry the plates after washing, protect the strip plates from falling.
5. The optimal assay results may only be achieved by strictly following the instructions and using only the reagents provided in the kit.
6. Please timely replace reagent troughs and pipette tips when loading different samples and performing

different steps, so as to avoid cross contamination.

7. The final assay results are closely related to reagent effectiveness, the operations of analysts, and the test environment.
8. Our company is only responsible for the kits themselves, and will not be responsible for the sample consumption caused by kits during use. Users should fully consider the possible sample consumption before operation, and should reserve sufficient sample size.

Safety reminder

1. The stop solution in this kit is acidic, thus extra attention should be paid during operation.
2. All biological samples may cause potential biosafety risks, therefore, users must strictly follow local laws and regulations when handling and disposing of the samples.
3. For safety concern, the operators should wear personal protective equipment such as lab coat, gloves, mask, and safety glasses.