



User's Manual

Human T-cell lymphotropic Virus antibody, HTLV (1+2) Ab ELISA Kit

REF

DEIA079



96T

RUO

This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

Creative Diagnostics

 **Address:** 45-1 Ramsey Road, Shirley, NY 11967, USA

 **Tel:** 1-631-624-4882 (USA) 44-161-818-6441 (Europe)  **Fax:** 1-631-938-8221

 **Email:** info@creative-diagnostics.com  **Web:** www.creative-diagnostics.com

PRODUCT INFORMATION

Intended Use

This ELISA kit is an enzyme-linked immunosorbent assay (ELISA) for qualitative detection of antibodies to Human T-Cell Lymphotropic Virus types 1 and/or 2 (HTLV-1/2) in human serum or plasma.

General Description

The human T-cell lymphotropic viruses (HTLV) is a member of the family of Retroviridae, consisting of enveloped double stranded RNA viruses and genetically not related to HIV1&2; however, they have similar routes of transmission and can have extremely long period of latency prior to manifestation of disease. HTLV type 1 was reported in 1980 as the first retrovirus shown to be pathogenic to humans. The virus preferentially infects CD4+ lymphocytes while the infections of CD8+ T lymphocytes are rare. In contrast to HTLV 1, HTLV type 2 can infect all type of lymphocytes as well as the macrophages. HTLV 1&2 is transmitted transplacentally, parenterally, by sexual contacts and by infected blood. The diseases associated with HTLV infection are usually classified as malignant or nonmalignant clinical presentations. HTLV 1 is endemic in southern Japan, the Caribbean and the US and many other scattered population through the world. HTLV 2 is endemic in some North American Indian tribes but is detected mostly in intravenous drug users and their sexual partners.

Principles of Testing

This kit uses one-step incubation, antigen "sandwich" enzyme immunoassay (ELISA) method, which uses polystyrene microwell strips pre-coated with recombinant HTLV antigens expressed in E.coli. Patient's serum/plasma sample is incubated in the microwells together with second recombinant HTLV antigens conjugated to horseradish peroxidase (HRP-Conjugate). The pre-coated antigens express the same epitopes as the HRP-Conjugate antigens, but are expressed in different hosts. In case of presence of anti-HTLV in sample, the pre-coated and HRP-conjugated antigens will be bound to the two variable domains of the antibody and during incubation, the specific antigen-antibody immunocomplex is captured on the solid phase. After washing to remove sample and unbound HRP-Conjugate, Chromogen solutions containing tetramethylbenzidine (TMB) and urea peroxide are added to the wells. In presence of the antigen-antibody-antigen (HRP) "sandwich" complex, the colorless Chromogens are hydrolyzed by the bound HRP-Conjugate to a blue-colored product. The blue color turns yellow after stopping the reaction with sulfuric acid. The amount of color intensity can be measured and is proportional to the amount of antibody captured in the wells, and to the sample respectively. Wells containing samples negative for anti-HTLV remain colorless.

Reagents And Materials Provided

1. MICROWELL PLATE: 12x8 wells. Blank microwell strips fixed on white strip holder. The plate is sealed in aluminum pouch with desiccant. Each well contains recombinant HTLV 1/2 antigens. The microwell strips can be broken to be used separately. Place unused wells or strips in the provided plastic sealable storage bag together with the desiccant and return to 2-8°C. Once open, stable for one month at 2-8°C.

2. NEGATIVE CONTROL: 1x0.5ml per vial. preserv. 0.1% ProClin 300. Yellowish liquid filled in a vial with green screw cap. Protein-stabilized buffer tested non reactive for anti-HTLV 1/2. Ready to use as supplied.

Once open, stable for one month at 2-8°C.

3. POSITIVE CONTROL: 1x0.5ml per vial. preserv. 0.1% ProClin 300. Red-colored liquid filled in a vial with red screw cap. Antibodies to HTLV 1/2 diluted in protein-stabilized buffer. Ready to use as supplied. Once open, stable for one month at 2-8°C.

4. HRP-CONJUGATE: 1x6ml per bottle. Red-colored liquid in a white vial with red screw cap. Horseradish peroxidase-conjugated HTLV 1/2 antigens. Ready to use as supplied. Once open, stable for one month at 2-8°C.

5. WASH BUFFER: 1x50ml per bottle. preserv. 0.1% ProClin 300. Colorless liquid filled in a white bottle with white screw cap. PH 7.4, 20 x PBS The concentrate must be diluted 1 to 20 with distilled/deionized water before use. Once diluted, stable for one week at room temperature, or for two weeks when stored at 2-8°C

6. CHROMOGEN SOLUTION A: 1x7ml per vial. Colorless liquid filled in a white vial with green screw cap. Urea peroxide solution. Ready to use as supplied. Once open, stable for one month at 2-8°C.

7. CHROMOGEN SOLUTION B: 1x7ml per vial. Colorless liquid filled in a black vial with black screw cap. TMB (Tetramethyl benzidine) solution. Ready to use as supplied. Once open, stable for one month at 2-8°C.

8. STOP SOLUTION: 1x7ml per vial. Colorless liquid in a white vial with white screw cap. Diluted sulfuric acid solution (0.5M H₂SO₄). Ready to use as supplied. Once open, stable for one month at 2-8°C.

Materials Required But Not Supplied

Freshly distilled or deionized water, disposable gloves and timer, appropriate waste containers for potentially contaminated materials, dispensing system and/or pipette, disposable pipette tips, absorbent tissue or clean towel, dry incubator or water bath, 37±0.5°C, plate reader, single wavelength 450nm or dual wavelength 450/630nm, microwell aspiration/wash system.

Storage

The components of the kit will remain stable through the expiration date indicated on the label and package when stored between 2-8°C, do not freeze. To assure maximum performance of this ELISA kit, during storage, protect the reagents from contamination with microorganism or chemicals.

Specimen Collection And Preparation

1. Specimen Collection: No special patient's preparation required. Collect the specimen in accordance with the normal laboratory practice. Either fresh serum or plasma specimens can be used with this assay. Blood collected by venipuncture should be allowed to clot naturally and completely – the serum/plasma must be separated from the clot as early as possible as to avoid haemolysis of the RBC. Care should be taken to ensure that the serum specimens are clear and not contaminated by microorganisms. Any visible particulate matters in the specimen should be removed by centrifugation at 3000 RPM (round per minutes) for 20 minutes at room temperature or by filtration.
2. Plasma specimens collected into EDTA, sodium citrate or heparin can be tested, but highly lipaemic, icteric, or hemolytic specimens should not be used as they can give false results in the assay. Do not heat inactivate specimens. This can cause deterioration of the target analyte. Samples with visible microbial contamination should never be used.

3. This ELISA kit is intended ONLY for testing of individual serum or plasma samples. Do not use the assay for testing of cadaver samples, saliva, urine or other body fluids, or pooled (mixed) blood.
4. Transportation and Storage: Store specimens at 2-8°C. Specimens not required for assaying within 7 days should be stored frozen (-20°C or lower). Multiple freeze-thaw cycles should be avoided. For shipment, samples should be packaged and labeled in accordance with the existing local and international regulations for transportation of clinical samples and ethological agents.

Reagent Preparation

Reagents preparation: Allow the reagents to reach room temperature (18-30°C). Check the Wash buffer concentrate for the presence of salt crystals. If crystals have formed, resolubilize by warming at 37°C until crystals dissolve. Dilute the Wash buffer (20×) as indicated in the instructions for washing. Use distilled or deionized water and only clean vessels to dilute the buffer. All other reagents are READY TO USE AS SUPPLIED.

Assay Procedure

1. Preparation: Mark three wells as Negative control (e.g. B1, C1, D1), two wells as Positive control (e.g. E1, F1) and one Blank (e.g. A1, neither samples nor HRP-Conjugate should be added into the Blank well). If the results will be determined by using dual wavelength plate reader, the requirement for use of Blank well could be omitted. Use only number of strips required for the test.
2. Adding HRP-Conjugate: Add 50µl of HRP-Conjugate into each well except the Blank.
3. Adding Sample: Add 50µl of Positive control, Negative control, and Specimen into their respective wells except the Blank. **Note: Use a separate disposal pipette tip for each specimen and standard to avoid cross-contamination. Mix by tapping the plate gently.**
4. Incubating: Cover the plate with the plate cover and incubate for 60 minutes at 37°C.
5. Washing: At the end of the incubation, remove and discard the plate cover. Wash each well 5 times with diluted Wash Buffer. Each time allow the microwells to soak for 30-60 seconds. After the final washing cycle, turn down the plate onto blotting paper or clean towel and tap it to remove any remainders.
6. Coloring: Add 50µl of Chromogen A and 50µl of Chromogen B solutions into each well including the Blank. Incubate the plate at 37°C for 30 minutes avoiding light. The enzymatic reaction between the Chromogen solutions and the HRP-Conjugate produces blue color in Positive control and in anti-HTLV 1/2 positive sample wells.
7. Stopping Reaction: Using a multichannel pipette or manually, add 50µl of Stop Solution into each well and mix gently. Intensive yellow color develops in Positive control and anti-HTLV 1/2 positive sample wells.
8. Measuring the Absorbance: Calibrate the plate reader with the Blank well and read the absorbance at 450nm. If a dual filter instrument is used, set the reference wavelength at 630nm. Calculate the Cut-off value and evaluate the results. **(Note: read the absorbance within 10 minutes after stopping the reaction).**

Washing Notes:

1. A good washing procedure is essential in order to obtain correct and precise analytical data.
2. It is therefore, recommended to use a good quality ELISA microplate washer, maintained at the best level of washing performances. In general, no less than 5 automatic washing cycles of 350-400µl/well are sufficient

to avoid false positive reactions and high background.

- To avoid cross-contaminations of the plate with specimen or HRP-conjugate, after incubation, do not discard the content of the wells but allow the plate washer to aspirate it automatically.
- Assure that the microplate washer liquid dispensing channels are not blocked or contaminated and sufficient volume of Wash buffer is dispensed each time into the wells.
- In case of manual washing, we suggest to carry out 5 washing cycles, dispensing 350-400µl/well and aspirating the liquid for 5 times. If poor results (high background) are observed, increase the washing cycles or soaking time per well.
- In any case, the liquid aspirated out the strips should be treated with a sodium hypochlorite solution at a final concentration of 2.5% for 24 hours, before they are wasted in an appropriate way.
- The concentrated Wash buffer should be diluted 1 to 20 before use. If less than a whole plate is used, prepare the proportional volume of solution.

Quality Control

Each microplate should be considered separately when calculating and interpreting the results of the assay, regardless of the number of plates concurrently processed. The results are calculated by relating each specimen absorbance (A) value to the Cut-off value (C.O.) of the plate. If the Cut-off reading is based on single filter plate reader, the results should be calculated by subtracting the Blank well A value from the print report values of specimens and controls. In case the reading is based on dual filter plate reader, do not subtract the Blank well A value from the print report values of specimens and controls.

Calculation of the Cut-off value (C.O.) = $N_c + 0.18$ (N_c = the mean absorbance value for three negative controls).

Quality control (assay validation): The test results are valid if the Quality Control criteria are fulfilled. It is recommended that each laboratory must establish appropriate quality control system with quality control material similar to or identical with the patient sample being analyzed.

The A value of the Blank well, which contains only Chromogen and Stop solution, is < 0.080 at 450 nm.

The A values of the Positive control must be ≥ 0.800 at 450/630nm or at 450nm after blanking.

The A values of the Negative control must be < 0.100 at 450/630nm or at 450nm after blanking.

If one of the Negative control A values does not meet the Quality Control criteria, it should be discarded and the mean value calculated again using the remaining two values. If more than one Negative control A values do not meet the Quality Control Range specifications, the test is invalid and must be repeated.

Example:

1. Quality Control

Blank well A value: A1= 0.025 at 450nm (Note: blanking is required only when reading with single filter at 450nm)

Well No.:	B1	C1	D1
Negative control A values after blanking:	0.028	0.030	0.032
Well No.:	E1	F1	
Positive control A values after blanking:	2.421	2.369	

All control values are within the stated quality control range

2. Calculation of N_c : = $\frac{(0.028+0.030+0.032)}{3}$ = 0.030

3. Calculation of the Cut-off: (C.O.) = $0.030 + 0.18$ = 0.210

Interpretation Of Results


Negative Results (A / C.O. < 1): Specimens giving absorbance less than the Cut-off value are negative for this assay, which indicates that no antibodies to HTLV 1/2 has been detected with this ELISA kit. Therefore,

the patient is probably not infected with HTLV 1/2.

Positive Results ($A / C.O. \geq 1$): Specimens giving an absorbance equal to or greater than the Cut-off value are considered initially reactive, which indicates that antibodies to HTLV 1/2 has probably been detected using this ELISA kit. All initially reactive specimens should be retested in duplicates using this ELISA kit before the final assay results interpretation. Repeatedly reactive specimens could be considered positive for antibodies to HTLV 1/2 and therefore there are serological indications for infection with HTLV 1/2.

Borderline ($A / C.O. = 0.9-1.1$): Specimens with absorbance to Cut-off ratio between 0.9 and 1.1 are considered borderline and retesting of these specimens in duplicates is required to confirm the initial results.

Follow-up, confirmation and supplementary testing of any positive specimen with other analytical system is required. Clinical diagnosis should not be established based on a single test result. It should integrate clinical and other laboratory data and findings.

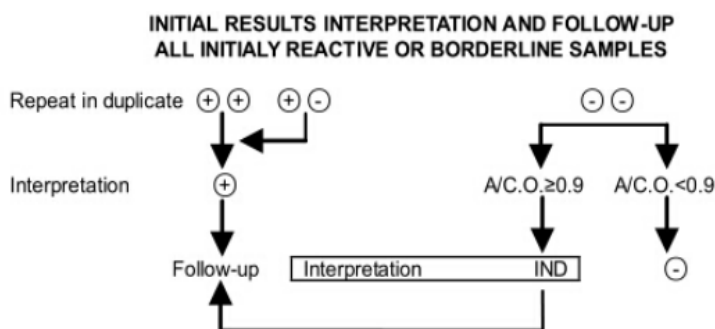

IND = non interpretable

a. If, after retesting of the initially reactive samples, both wells are negative results ($A/C.O. < 0.9$), these samples should be considered as non-repeatable positive (or false positive) and recorded as negative. As with many very sensitive ELISA assays, false positive results can occur due to the several reasons, most of which are connected with, but not limited to, inadequate washing step.

b. If after retesting in duplicates, one or both wells are positive results, the final result from this ELISA test should be recorded as repeatedly reactive. Repeatedly reactive specimens could be considered positive for antibodies to HTLV 1/2.

c. After retesting in duplicates, samples with values close to the Cut-off value should be interpreted with caution and considered as "borderline" zone sample, or uninterpretable for the time of testing.

Performance Characteristics

The clinical performances of this assay have been evaluated by a panel of samples obtained from 22145 healthy blood donors from 3 blood banks and by a panel of samples from 125 HTLV 1/2 positive patients (105 HTLV 1 and 20 HTLV 2 samples from patients with well characterized clinical history and confirmed Western Blot and PCR positive results). The evaluation results are given below.

Sample	Number of Sample	-	+	Confirmed	Sensitivity	False Negative
HTLV-1	105	0	105	105	100%	0
HTLV-2	20	0	20	20	100%	0

Donors	Number of Sample	-	+	Confirmed	Specificity	False Positive
Location 1*	4103	4101	2	0	99.95%	2
Location 2*	15044	15042	2	0	99.99%	2
Location 3*	2998	2998	0	/	100%	0
Total	22145	22141	4	0	99.98%	4

Performance on BBI anti-HTLV panel:

Reagent		EIA1	EIA2	EIA3	EIA4	This kit	EIA5	
Member	HTLV	I/II	I/II	I/II	I/II	I/II	I	II
I.D#	Type	s/co	s/co	s/co	s/co	s/co	s/co	s/co
PRB205-01	I	> 4.0	> 15.2	4.0	5.77	12.68	> 17.4	> 13.8
PRB205-02	II	3.3	4.8	1.9	1.65	11.81	0.4	6.2
PRB205-03	II	> 4.0	2.9	3.3	3.17	13.32	0.3	12.0
RPB205-04	II	> 4.0	> 15.2	4.2	5.85	13.26	0.4	> 13.8
PRB205-05	II	> 4.0	> 15.2	4.3	5.90	13.32	0.2	> 13.8
PRB205-06	NEG	0.2	0.1	0.1	0.03	0.02	0.1	0.2
PRB205-07	I	> 4.0	10.2	3.3	3.02	13.48	3.5	0.5
PRB205-08	II	> 4.0	4.4	3.1	2.11	13.48	0.2	3.3
PRB205-09	II	> 4.0	> 15.2	3.6	5.24	12.9	0.2	> 13.8
PRB205-10	II	> 4.0	1.3	3.3	2.01	13.30	0.0	1.3
PRB205-11	I	> 4.0	3.0	2.6	4.32	12.91	2.2	0.3
PRB205-12	I	> 4.0	> 15.2	4.1	6.19	12.43	> 17.4	2.7
PRB205-13	II	> 4.0	5.0	2.6	1.03	10.00	0.2	6.3
PRB205-14	I	> 4.0	7.2	3.3	5.07	12.7	4.8	0.3
PRB205-15	I	> 4.0	13.9	2.5	5.90	19.41	16.0	0.3
PRB205-16	II	> 4.0	12.9	4.2	1.38	13.91	0.2	13.2
PRB205-17	I	> 4.0	> 15.2	3.5	6.51	14.25	> 17.4	0.9
PRB205-18	II	> 4.0	2.5	2.6	3.13	14.32	0.2	2.7
PRB205-19	I	> 4.0	12.1	1.9	3.10	10.94	14.0	0.4
PRB205-20	I	> 4.0	> 15.2	4.2	5.63	13.36	17.4	1.4
PRB205-21	I	> 4.0	1.6	3.0	1.30	10.16	0.1	1.0
PRB205-22	II	> 4.0	1.7	2.2	0.64	8.36	0.1	2.5
PRB205-23	II	> 4.0	1.5	3.1	0.53	8.62	0.0	1.1
PRB205-24	NEG	0.3	0.1	0.1	0.04	0.022	0.1	0.4
PRB205-25	I	> 4.0	> 15.2	4.2	5.67	14.11	> 17.4	2.9

Performance on Pasteur Institute anti-HTLV panel:

HTLV	EIA HTLV I/II	This HTLV I/II
Type	s/co	s/co
I	5.52	11.30
I	5.29	13.19
II	3.88	12.60
I	5.59	12.04
I	5.30	12.35
I	5.91	3.07
I	5.80	11.80
I	5.78	12.31
I	6.04	11.75
II	5.60	9.74
II	1.15	12.02
II	2.17	11.91

Specificity

No cross reactivity was observed with specimens from patients infected with HAV, HCV, HBV, HIV, CMV and TP. No interference was observed from rheumatoid factors up to 2000U/ml. No high dose hook effect observed during clinical testing. The assay performance characteristics are unaffected from elevated concentrations of bilirubin, hemoglobin, and triolein. Frozen specimens have been tested to check for interferences due to collection and storage.

Precautions

The ELISA assays are time and temperature sensitive. To avoid incorrect result, strictly follow the test procedure steps and do not modify them.

- Do not exchange reagents from different lots or use reagents from other commercially available kits. The components of the kit are precisely matched for optimal performance of the tests.

2. Make sure that all reagents are within the validity indicated on the kit box and of the same lot. Never use reagents beyond their expiry date stated on labels or boxes.
3. **CAUTION - CRITICAL STEP:** Allow the reagents and specimens to reach room temperature (18-30°C) before use. Shake reagent gently before use. Return at 2-8°C immediately after use.
4. Use only sufficient volume of sample as indicated in the procedure steps. Failure to do so, may cause in low sensitivity of the assay.
5. Do not touch the bottom exterior of the wells; fingerprints or scratches may interfere with the reading. When reading the results, ensure that the plate bottom is dry and there are no air bubbles inside the wells.
6. Never allow the microplate wells to dry after the washing step. Immediately proceed to the next step. Avoid the formation of air bubbles when adding the reagents.
7. Avoid assay steps long time interruptions. Assure same working conditions for all wells.
8. Calibrate the pipette frequently to assure the accuracy of samples/reagents dispensing. Use different disposal pipette tips for each specimen and reagents in order to avoid cross-contaminations.
9. Assure that the incubation temperature is 37°C inside the incubator.
10. When adding specimens, do not touch the well's bottom with the pipette tip.
11. When measuring with a plate reader, determine the absorbance at 450nm or at 450/630nm.
12. The enzymatic activity of the HRP-conjugate might be affected from dust and reactive chemical and substances like sodium hypochlorite, acids, alkalis etc. Do not perform the assay in the presence of these substances.
13. If using fully automated equipment, during incubation, do not cover the plates with the plate cover. The tapping out of the remainders inside the plate after washing, can also be omitted.
14. All specimens from human origin should be considered as potentially infectious. Strict adherence to GLP (Good Laboratory Practice) regulations can ensure the personal safety.
15. **WARNING:** Materials from human origin may have been used in the preparation of the Negative Control of the kit. These materials have been tested with tests kits with accepted performance and found negative for antibodies to HIV 1/2, HCV, TP and HBsAg. However, there is no analytical method that can assure that infectious agents in the specimens or reagents are completely absent. Therefore, handle reagents and specimens with extreme caution as if capable of transmitting infectious diseases. Bovine derived sera have been used for stabilizing of the positive and negative controls. Bovine serum albumin (BSA) and fetal calf sera (FCS) are derived from animals from BSE/TSE free-geographical areas.
16. Never eat, drink, smoke, or apply cosmetics in the assay laboratory. Never pipette solutions by mouth.
17. Chemical should be handled and disposed of only in accordance with the current GLP (Good Laboratory Practices) and the local or national regulations.
18. The pipette tips, vials, strips and specimen containers should be collected and autoclaved for not less than 2 hours at 121°C or treated with 10% sodium hypochlorite for 30 minutes to decontaminate before any further steps of disposal. Solutions containing sodium hypochlorite should NEVER be autoclaved. Materials Safety Data Sheet (MSDS) available upon request.
19. Some reagents may cause toxicity, irritation, burns or have carcinogenic effect as raw materials. Contact with the skin and the mucosa should be avoided but not limited to the following reagents: Stop solution, the Chromogens, and the Wash buffer.
20. The Stop solution 0.5M H₂SO₄ is an acid. Use it with appropriate care. Wipe up spills immediately and wash with water if come into contact with the skin or eyes.



21. ProClin 300 0.1% used as preservative, can cause sensation of the skin. Wipe up spills immediately or wash with water if come into contact with the skin or eyes.

INDICATIONS OF INSTABILITY DETERIORATION OF THE REAGENT: Values of the Positive or Negative controls, which are out of the indicated quality control range, are indicators of possible deterioration of the reagents and/or operator or equipment errors. In such case, the results should be considered as invalid and the samples must be retested. In case of constant erroneous results and proven deterioration or instability of the reagents, immediately substitute the reagents with new one.

Limitations

1. Positive results must be confirmed with another available method and interpreted in conjunction with the patient clinical information.
2. Antibodies may be undetectable during the early stage of the disease and in some immunosuppressed individuals. Therefore, negative results obtained with this ELISA kit are only indication that the sample does not contain detectable level of anti-HTLV 1/2 antibodies and any negative result should not be considered as conclusive evidence that the individual is not infected with HTLV 1/2.
3. If, after retesting of the initially reactive samples, the assay results are negative, these samples should be considered as nonrepeatable (false positive) and interpreted as negative. As with many very sensitive ELISA assays, false positive results can occur due to the several reasons, most of which are related but not limited to inadequate washing step.
4. The most common assay mistakes are: using kits beyond the expiry date, bad washing procedures, contaminated reagents, incorrect assay procedure steps, insufficient aspiration during washing, failure to add specimens or reagents, improper operation with the laboratory equipment, timing errors, the use of highly hemolyzed specimens or specimens containing fibrin, incompletely clotted serum specimens.
5. The prevalence of the marker will affect the assay's predictive values.
6. This kit is intended **ONLY** for testing of individual serum or plasma samples. Do not use it for testing of cadaver samples, saliva, urine or other body fluids, or pooled (mixed) blood.
7. The assay cannot distinguish between infections with HTLV-1 and HTLV-2.
8. This kit is a qualitative assay and the results cannot be used to measure antibodies concentrations.